



WORKSHOP PRESENTATION

Open Access

Segmented CMR acquisition with iterative SENSE reconstruction using L1-regularization in the evaluation of right ventricular systolic function

Abraham Bogachkov^{1*}, Maria Carr¹, Bradley D Allen², Marie Wasielewski², Karissa Campione², Bruce S Spottiswoode³, Michaela Schmidt⁴, Michael O Zenge⁴, Mariappan S Nadar⁵, James C Carr², Jeremy D Collins²

From 17th Annual SCMR Scientific Sessions
 New Orleans, LA, USA. 16-19 January 2014

Background

Cardiac MR (CMR) has emerged as the gold standard in assessing biventricular size and systolic function with segmented balanced steady-state free-precession (bSSFP) cine acquisitions. The application of a novel prototype iterative reconstruction technique to sparsely under-sampled segmented bSSFP cine acquisitions may enable higher acceleration factors while shortening image acquisitions, thus maintaining adequate image quality for quantitative analysis. The purpose of this study is to evaluate the clinical utility of a segmented sparsely sampled 2D CINE imaging technique, with a prototype iterative SENSE reconstruction using L1-regularization, in the quantitative assessment of right ventricular (RV) systolic function.

Methods

9 healthy volunteers (44.3 ± 13.5 yrs) and 29 patients (54.3 ± 13.8 yrs) with suspected cardiac pathology were scanned on a 1.5T scanner (MAGNETOM Aera, Siemens AG, Healthcare Sector, Erlangen, Germany). All subjects were imaged using a conventional segmented bSSFP cine sequence with GRAPPA factor 2 acceleration ("CINE Seg", temp res = 40 msec, 25 phases, slice = 6 mm, in-plane res = 1.5×1.5 mm², acq time 8.4 sec) and a segmented in-plane sparsely sampled acquisition with T-PAT factor 4 acceleration and prototype iterative SENSE reconstruction using L1-regularization ("CINE Seg-IR", eff temp res = 39 msec, 20 phases, slice = 6 mm, in-plane res = 1.9×1.8 mm², acq time 4 sec). Quantitative

RV systolic function analysis was performed by a single reviewer on a dedicated workstation (QMass 5.2, Medis, Leiden, Netherlands). Continuous variables were analyzed using linear regression. A blinded reviewer scored images for overall image quality, noise, and artifacts using a 5-point Likert scale. 14 patients were re-analyzed to evaluate intraobserver agreement using the intraclass correlation coefficient (ICC).

Results

Acceptable CINE Seg-IR acquisitions were successfully acquired in all subjects. The mean difference in ejection fraction (EF) and indexed stroke volume (SV) between CINE Seg and CINE Seg-IR were $-0.02 \pm 3.74\%$ and 0.18 ± 3.76 mL/m², respectively. The R² value for linear regression of CINE Seg-IR versus CINE Seg is shown in Figure 1. Qualitative review yielded comparable values for CINE SEG versus CINE Seg-IR, as seen in Table 1. ICC values for CINE Seg and CINE Seg-IR, were 0.878 and 0.941 for EF, and 0.955 and 0.922 for SV, respectively.

Conclusions

Segmented sparsely sampled cine bSSFP imaging with T-PAT factor 4 and iterative SENSE reconstruction using L1-regularization at 1.5T can both accurately and reliably quantitate RV systolic function parameters as compared to conventional segmented cine sequences with GRAPPA factor 2 acceleration. This technique has the potential to shorten examination times by 50% while improving imaging options in patients with arrhythmias or difficulty with breath-holding.

¹Northwestern University, Feinberg School of Medicine, Chicago, Illinois, USA
 Full list of author information is available at the end of the article

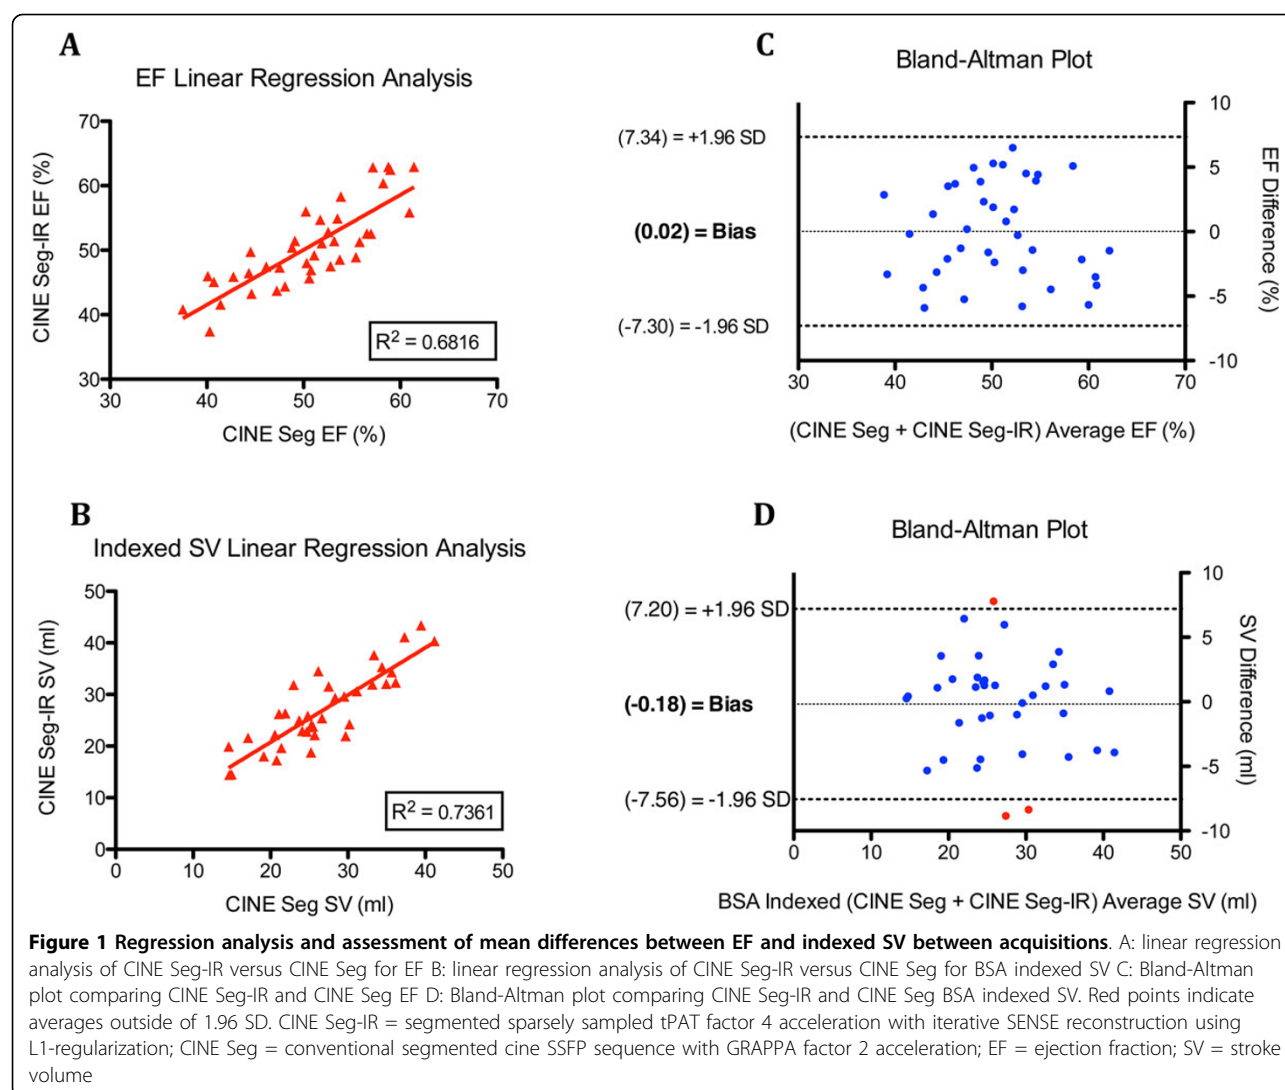


Table 1 Qualitative scoring in the combined cohort of patients and volunteers.

Image Acquisition	Quality	Noise	Artifact
CINE Seg	4.8 ± 0.4*	4.9 ± 0.3*	4.8 ± 0.4*
CINE Seg-IR	4.6 ± 0.6*	4.6 ± 0.6*	4.6 ± 0.6*

* = p-value < 0.05 relative to CINE Seg-IR

Funding

Northwestern University, Feinberg School of Medicine, AOSC Grant.

Authors' details

¹Northwestern University, Feinberg School of Medicine, Chicago, Illinois, USA. ²Radiology, Northwestern University, Chicago, Illinois, USA. ³Cardiovascular MR R&D, Siemens Healthcare, Chicago, Illinois, USA. ⁴Siemens AG, Healthcare Sector, Erlangen, Germany. ⁵Corporate Technology, Siemens Corporation, Princeton, New Jersey, USA.

Published: 16 January 2014

doi:10.1186/1532-429X-16-S1-W17

Cite this article as: Bogachkov et al.: Segmented CMR acquisition with iterative SENSE reconstruction using L1-regularization in the evaluation of right ventricular systolic function. *Journal of Cardiovascular Magnetic Resonance* 2014 **16**(Suppl 1):W17.

Submit your next manuscript to BioMed Central and take full advantage of:

- Convenient online submission
- Thorough peer review
- No space constraints or color figure charges
- Immediate publication on acceptance
- Inclusion in PubMed, CAS, Scopus and Google Scholar
- Research which is freely available for redistribution

Submit your manuscript at
www.biomedcentral.com/submit

